

Human calprotectin ELISA Kit

USER INSTRUCTION

Cat.No BTB-E4010hu

Standard Curve Range: 2-600ng/ml

Sensitivity: 1.67ng/ml

Size: 96 wells / 48 wells

Storage: Store the reagents at 2-8°C. For over 6-month storage refer to the expiration date keep it at -20°C. Avoid repeated thaw cycles. If individual reagents are opened it is recommended that the kit be used within 1 month.

***This product is for research use only, not for use in diagnosis procedures. It's highly recommended to read this instruction entirely before use.**

Precision

Intra-Assay Precision (Precision within an assay) Three samples of known concentration were tested on one plate to assess intra-assay precision.

Inter-Assay Precision (Precision between assays) Three samples of known concentration were tested in separate assays to assess inter-assay precision.

$CV(\%) = SD/mean \times 100$

Intra-Assay: $CV < 8\%$

Inter-Assay: $CV < 10\%$

Intended Use

This sandwich kit is for the accurate quantitative detection of Human calprotectin (also known as CAL) in serum, plasma, urine, feces, cell culture supernates, tissue homogenates, other related tissue Liquid.

Assay Principle

This kit is an Enzyme-Linked Immunosorbent Assay (ELISA). The plate has been pre-coated with Human CAL antibody. CAL present in the sample is added and binds to antibodies coated on the wells. And then biotinylated Human CAL Antibody is added and binds to CAL in the sample. Then Streptavidin-HRP is added and binds to the Biotinylated CAL antibody. After incubation unbound

Streptavidin-HRP is washed away during a washing step. Substrate solution is then added and color develops in proportion to the amount of Human CAL. The reaction is terminated by addition of acidic stop solution and absorbance is measured at 450 nm.

Reagent Provided

| Components | Quantity (96T) | Quantity (48T) |
|---------------------------------|-----------------------|-----------------------|
| Standard Solution (640ng/ml) | 0.5ml x1 | 0.5ml x1 |
| Pre-coated ELISA Plate | 12 * 8 well strips x1 | 12 * 4 well strips x1 |
| Standard Diluent | 3ml x1 | 3ml x1 |
| Streptavidin-HRP | 6ml x1 | 3ml x1 |
| Stop Solution | 6ml x1 | 3ml x1 |
| Substrate Solution A | 6ml x1 | 3ml x1 |
| Substrate Solution B | 6ml x1 | 3ml x1 |
| Wash Buffer Concentrate (25x) | 20ml x1 | 20ml x1 |
| Biotinylated Human CAL Antibody | 1ml x1 | 1ml x1 |
| User Instruction | 1 | 1 |
| Plate Sealer | 2 pics | 2 pics |
| Zipper bag | 1 pic | 1 pic |

Material Required But Not Supplied

- 37°C±0.5°C incubator
- Absorbent paper
- Precision pipettes and disposable pipette tips
- Clean tubes
- Deionized or distilled water
- Microplate reader with 450 ± 10nm wavelength filter

Precautions

- Prior to use, the kit and sample should be warmed naturally to room temperature 30 minutes.
- This instruction must be strictly followed in the experiment.
- Once the desired number of strips has been removed, immediately reseal the bag to protect the remain from deterioration. Cover all reagents when not in use.
- Make sure pipetting order and rate of addition from well-to-well when pipetting reagents.
- Pipette tips and plate sealer in hand should be clean and disposable to avoid cross-contamination.
- Avoid using the reagents from different batches together.

- Substrate solution B is sensitive to light, don't expose substrate solution B to light for a long time.
- Stop solution contains acid. Please wear eye, hand and skin protection when using this material. Avoid contact of skin or mucous membranes with kit reagent.
- The kit should not be used beyond the expiration date.

Specimen Collection

Serum Allow serum to clot for 10-20 minutes at room temperature. Centrifuge at 2000-3000 RPM for 20 minutes. Collect the supernatant without sediment.

Plasma Collect plasma using EDTA or heparin as an anticoagulant. After mix 10-20 minutes, centrifuge samples for 20 minutes at 2000-3000 RPM. Collect the supernatant without sediment.

Urine/Ascites/ Cerebrospinal fluid Collect by sterile tube. Centrifuge at 2000-3000 RPM for 20 minutes. Collect the supernatant without sediment.

Cell culture supernatant Collect by sterile tubes. When detecting secreted components, centrifuge at 2000-3000 RPM for 20 minutes. Collect the supernatants. When detecting the components in the cell, use PBS (pH 7.2-7.4) to dilute cell suspension, the cell concentration of approximately 1 million/ml. Damage cells through repeated freeze-thaw cycles to let out the inside components. Centrifuge at 2000-3000 RPM for 20 minutes. Collect the supernatant without sediment.

Tissue Rinse tissues in ice-cold PBS (pH 7.4) to remove excess blood thoroughly and weigh before homogenization. Mince tissues and homogenize them in PBS (tissue weight (g): PBS (mL) volume=1:9) with a glass homogenizer on ice. To further break down the cells, you can sonicate the suspension with an ultrasonic cell disrupter or subject it to freeze-thaw cycles. The homogenates are then centrifuged for 5 minutes at 5000×g to get the supernatant.

Solid samples (feces) Prepare with PBS (1g:9ml). Centrifuge at 2000-3000 RPM for approximately 20 minutes and collect the supernatant for assay.

Stool Detection of stool specimens to determine the digestive system diseases have important reference value. Collected with a clean bamboo sticks selected with mucus, pus and other abnormal components of the feces, the appearance of no abnormal faeces from the surface, deep and fecal multiple material. Find parasites and insect eggs count should be collected 24 hours feces. Check dysentery amoeba nourishing body should be checked immediately after defecation, from the pus and dilute the Department of materials, insulation inspection. Check the Japanese schistosomiasis eggs should take mucus, pus and blood part of the incubation of miracidia at least 30g of stool, and need to be treated as soon as possible. Check the pinworm eggs with a transparent film swab at 12 o'clock or early morning defecation before the anus around the folds at the wipe and immediately microscopic examination. Occult blood test (chemical method), 3 days before the test fasting meat and animal blood containing food and ban iron, vitamin C and so on. All fecal samples should be inspected within 1 hour after collection to prevent the destruction of visible components by digestive enzymes and pH. For example, 1g samples corresponding to the 9mL PBS, the specific volume can be adjusted according to the needs of the experiment, when the sample concentration is calculated after the test, the

dilution ratio should be multiplied.

1g stool sample +9ml PBS, 2g stool sample +18ml PBS

Note


- Sample concentrations should be predicted before being used in the assay. If the sample concentration is not within the range of the standard curve, users must **contact us** to determine the optimal sample for their particular experiments.
- Samples to be used within 5 days should be stored at 2-8°C. Samples should be aliquoted or must be stored at -20°C within 1 month or -80°C within 6 months. Avoid repeated freeze thaw cycles.
- Samples should be brought to room temperature before starting the assay.
- Centrifuge to collect sample before use.
- Samples containing NaN₃ can't be tested as it inhibits the activity of Horse Radish Peroxidase (HRP).
- Collect the supernatants carefully. When sediments occurred during storage, centrifugation should be performed again.
- Hemolysis can greatly impact the validity of test results. Take care to minimize hemolysis.

****Sample can't be diluted with this kit. Owing to the the material we use to prepare the kit, the sample matrix interference may falsely depress the specificity and accuracy of the assay.***

Reagent Preparation

- All reagents should be brought to room temperature before use.
- **Standard** Reconstitute the 120µl of the standard (640ng/ml) with 120µl of standard diluent to generate a 320ng/ml standard stock solution. Allow the standard to sit for 15 mins with gentle agitation prior to making dilutions. Prepare duplicate standard points by serially diluting the standard stock solution (320ng/ml) 1:2 with standard diluent to produce 160ng/ml, 80ng/ml, 40ng/ml and 20ng/ml solutions. Standard diluent serves as the zero standard(0 ng/ml). Any remaining solution should be frozen at -20°C and used within one month. Dilution of standard solutions suggested are as follows:

| | | |
|----------|---------------|--|
| 320ng/ml | Standard No.5 | 120µl Original Standard + 120µl Standard Diluent |
| 160ng/ml | Standard No.4 | 120µl Standard No.5 + 120µl Standard Diluent |
| 80ng/ml | Standard No.3 | 120µl Standard No.4 + 120µl Standard Diluent |
| 40ng/ml | Standard No.2 | 120µl Standard No.3 + 120µl Standard Diluent |
| 20ng/ml | Standard No.1 | 120µl Standard No.2 + 120µl Standard Diluent |

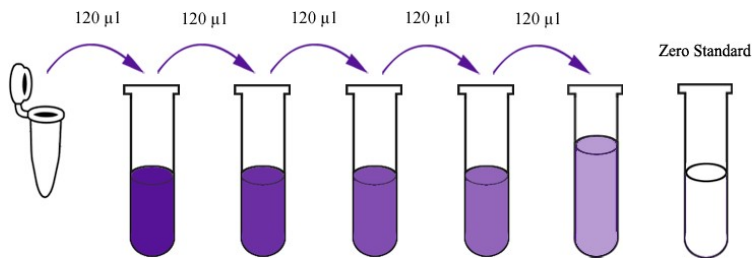

| Standard Concentration | Standard No.5 | Standard No.4 | Standard No.3 | Standard No.2 | Standard No.1 |
|------------------------|---------------|---------------|---------------|---------------|---------------|
| 640ng/ml | 320ng/ml | 160ng/ml | 80ng/ml | 40ng/ml | 20ng/ml |

- **Wash Buffer** Dilute 20ml of Wash Buffer Concentrate 25x into deionized or distilled water to yield 500 ml of 1x Wash Buffer. If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved.

Assay Procedure

1. Prepare all reagents, standard solutions and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature.
2. Determine the number of strips required for the assay. Insert the strips in the frames for use. The unused strips should be stored at 2-8°C.
3. Add 50µl standard to standard well. **Note:** Don't add biotinylated antibody to standard well because the standard solution contains biotinylated antibody.
4. Add 40µl sample to sample wells and then add 10µl anti-CAL antibody to sample wells, then add 50µl streptavidin-HRP to sample wells and standard wells (Not blank control well). Mix well. Cover the plate with a sealer. Incubate 60 minutes at 37°C.
5. Remove the sealer and wash the plate 5 times with wash buffer. Soak wells with 300ul wash buffer for 30 seconds to 1 minute for each wash. For automated washing, aspirate or decant each well and wash 5 times with wash buffer. Blot the plate onto paper towels or other absorbent material.
6. Add 50µl substrate solution A to each well and then add 50µl substrate solution B to each well. Incubate plate covered with a new sealer for 10 minutes at 37°C in the dark.
7. Add 50µl Stop Solution to each well, the blue color will change into yellow immediately.
8. Determine the optical density (OD value) of each well immediately using a microplate reader set to 450 nm within 10 minutes after adding the stop solution.

Summary

1. Prepare all reagents, samples and standards.
2. Add sample and ELISA reagent into each well. Incubate for 1 hour at 37°C.


3. Wash the plate 5 times.
4. Add substrate solution A and B. Incubate for 10 minutes at 37°C.
5. Add stop solution and color develops.
6. Read the OD value within 10 minutes.

Calculation of Result

Construct a standard curve by plotting the average OD for each standard on the vertical (Y) axis against the concentration on the horizontal (X) axis and draw a best fit curve through the points on the graph. These calculations can be best performed with computer-based curve-fitting software and the best fit line can be determined by regression analysis.

Typical Data

This standard curve is only for demonstration purposes. A standard curve should be generated with each assay.

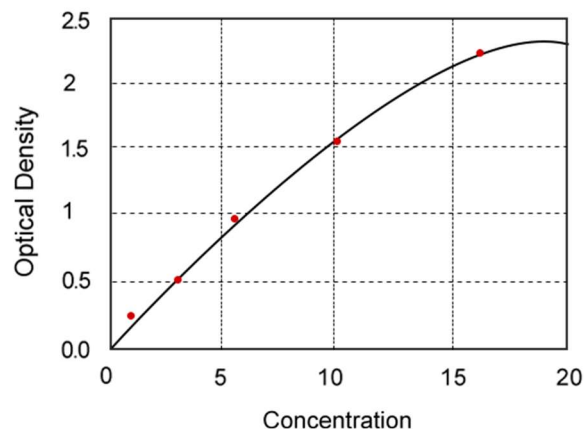

Troubleshooting

| Possible Case | Solution |
|--|--|
| High Background | |
| <ul style="list-style-type: none">• Improper washing• Substrate was contaminated• Non-specific binding of antibody• Plate are not be sealing incompletely• Incorrect incubation temperature• Substrate exposed to light prior to use• Contaminated wash buffer | <ul style="list-style-type: none">• Increasing duration of soaking steps• Replace. Substrate should be clean and avoid crossed contamination by using the sealer• Replace another purified antibody or blocking buffer• Make sure to follow the instruction strictly• Incubate at room temperature• Keep substrate in a dark place• Use a clean buffers and sterile filter |
| Weak Signal | |
| <ul style="list-style-type: none">• Improper washing• Incorrect incubation temperature• Antibody are not enough• Reagent are contaminated• Pipette are not clean | <ul style="list-style-type: none">• Increasing duration of soaking steps• Incubate at room temperature• Increase the concentration of the antibody• Use new one• Pipette should be clean |
| No Signal | |
| <ul style="list-style-type: none">• Reagent are contaminated• Sample prepared incorrectly• Antibody are not enough• Wash buffer contains sodium azide• HRP was not added | <ul style="list-style-type: none">• Use new one• Make sure the sample workable/dilution• Increase the antibody concentration• Use a new wash buffer and avoid sodium azide in it• Add HRP according to the instruction |
| Poor Precision | |
| <ul style="list-style-type: none">• Imprecise/ inaccurate pipetting• Incomplete washing of the wells | <ul style="list-style-type: none">• Check/ calibrate pipettes <p>Make sure wells are washed adequately by filling the wells with wash buffer and all residual antibody solutions crossed well before washing.</p> |