



EDI™ Quantitative Fecal/Urine NGAL ELISA Kit

Enzyme Linked ImmunoSorbent Assay (ELISA) for the Quantitative Measurement of Human Neutrophil Gelatinase-Associated Lipocalin Levels in Feces



INTENDED USE

This test kit is intended for use in the quantitative determination of human neutrophil gelatinase-associated lipocalin (Lipocalin-2 or NGAL) in feces. NGAL is extremely stable in feces.

Indications for use:

1. Patient may have an abnormally high level of NGAL in feces with active inflammatory bowel diseases (IBD), such as Crohn's disease, colitis ulcer, etc.
2. Patient may have an abnormally high level of NGAL in urine with acute kidney failure.

SUMMARY OF PHYSIOLOGY

NGAL or neutrophil gelatinase-associated lipocalin also known as Lipocalin-2 (LCN2) or oncogene 24p3 is a protein, which in humans is encoded by the *LCN2* gene.^{[1][2][3]} NGAL is involved in innate immunity by sequestering iron that in turn limits bacterial growth.^[4] It is expressed in neutrophils and in low levels in the kidney, prostate, and epithelia of the respiratory and alimentary tracts.^{[3][5]} Studies have shown that NGAL is an early biomarker for ischaemic renal injury after cardiopulmonary bypass.

ASSAY PRINCIPLE

This ELISA kit is designed, developed and produced for the quantitative measurement of human NGAL in stool samples. The assay utilizes the "sandwich" technique with selected antibodies that bind to various epitopes of NGAL.

Assay standards, controls and patient samples are added directly to wells of a microtiter plate that is coated with antibody to human NGAL and incubated at room temperature for one hour. The plate is then washed and horseradish peroxidase (HRP) conjugated anti-NGAL is added to each well. After an additional incubation period, a "sandwich" of solid-phase polyclonal antibody - human NGAL - HRP conjugated antibody is formed. The unbound antibodies and buffer matrix are removed in the subsequent washing step. For the detection of this immunocomplex, the well is then incubated with a substrate solution in a timed reaction, which is terminated with an acidic reagent (i.e. ELISA stop solution). The absorbance is then measured in a spectrophotometric microplate reader. The enzymatic activity of the immunocomplex bound to the wall of each microtiter well is directly proportional to the amount of human NGAL in the test sample. A standard curve is generated by plotting the absorbance versus the respective human NGAL concentration for each standard on a point-to-point or 4-parameter curve fitting. The concentration of human NGAL in test samples is determined directly from this standard curve.

REAGENTS: Preparation and Storage

This test kit must be stored at 2 – 8°C upon receipt. For the expiration date of the kit refer to the label on the kit box. All components are stable until this expiration date.

Prior to use allow all reagents to come to room temperature. Reagents from different kit lot numbers should not be combined or interchanged.

1. Anti-NGAL Antibody Coated Microplate (Cat. No. 30641)

One microplate with twelve by eight strips (96 wells total) coated with polyclonal anti-human NGAL antibody. The plate is framed and sealed in a foil zipper bag with a desiccant. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

2. HRP Conjugated Anti-NGAL Antibody (Cat. No. 30650)

One vial containing 0.6 mL HRP-labeled anti-human NGAL antibody in a stabilized protein matrix. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

3. ELISA Wash Concentrate (Cat. No. 10010)

One bottle containing 30 mL of 30-fold concentrate. Before use the contents must be diluted with 870 mL of demineralized water and mixed well. Upon dilution, this yields a working wash solution containing a surfactant in phosphate-buffered saline with a non-azide, non-mercury preservative. The diluted wash solution may be stored at room temperature and is stable until the expiration date on the kit box.

4. ELISA HRP Substrate (Cat. No. 10020)

One bottle containing 12 mL of tetramethylbenzidine (TMB) with hydrogen peroxide. This reagent should be stored at 2 – 8°C and is stable until the expiration date on the kit box.

5. ELISA Stop Solution (Cat. No. 10030)

One bottle containing 12 mL of stop solution. This reagent may be stored at 2 – 8°C or room temperature and is stable until the expiration date on the kit box.

6. Human NGAL Standards (Cat. No. 30642-30647)

Six vials containing recombinant human NGAL in a lyophilized bovine serum-based matrix with a non-azide preservative. **Refer to the vials for exact concentration of the standard.** These standards should be stored at 2 – 8°C and are stable until the expiration date on the kit box. Refer to assay procedure section for dilution direction.

7. Human NGAL Controls (Cat. No. 30648 – 30649)

Two vials containing human NGAL in a lyophilized bovine serum based matrix with a non-azide preservative. **Refer to vials for exact concentration range for each control.** Both controls should be stored at 2 – 8°C and are stable until the expiration date on the kit box. Refer to assay procedure section for reconstitution instructions.

8. Tracer Antibody Diluent (Cat. No. 30651)

One bottle containing 12 mL ready-to-use buffer. It should be used only for tracer antibody dilution according to the assay procedure. This reagent should be stored at 2 – 8 °C and is stable until the expiration date on the kit box.

9. Concentrated NGAL Fecal Extraction Buffer (Cat. No.30757)

One bottle containing 30 mL of 20-fold concentrate. Before use the contents must be diluted with 570 mL of demineralized water and mixed well. Upon dilution, this yields a ready-to-use Extraction Buffer for fecal sample extraction and dilution. The diluted Extraction Buffer may be stored at 2-8 °C and is stable for 2 months.

SAFETY PRECAUTIONS

The reagents must be used in professional laboratory. Source material for reagents containing bovine serum was derived in the contiguous 48 United States. It was obtained only from healthy donor animals maintained under veterinary supervision and found free of contagious diseases. Wear gloves while performing this assay and handle these reagents as if they are potentially infectious. Avoid contact with reagents containing TMB, hydrogen peroxide, or sulfuric acid. TMB may cause irritation to skin and mucous membranes and cause an allergic skin reaction. TMB is a suspected carcinogen. Sulfuric acid may cause severe irritation on contact with skin. Do not get in eyes, on skin, or on clothing. Do not ingest or inhale fumes. On contact, flush with copious amounts of water for at least 15 minutes. Use Good Laboratory Practices.

MATERIALS REQUIRED BUT NOT PROVIDED

1. Fecal sample collection tube (Epitope Catalog No: 30356)
2. Precision single channel pipettes capable of delivering 100 µL.
3. Disposable pipette tips suitable for above volume dispensing.
4. Aluminum foil.
5. Deionized or distilled water.
6. Plastic microtiter well cover or polyethylene film.
7. ELISA multichannel wash bottle or automatic (semi-automatic) washing system.
8. Spectrophotometric microplate reader capable of reading absorbance at 450/650 or 450/620 nm.

SPECIMEN COLLECTION

1. Only one fecal sample is required. Fresh fecal sample must be collected by using Epitope Diagnostics [Fecal Sample Collection Tube \(Cat. No. 30356\)](#). This tube is specially designed for easy collection of a substantially small amount of fecal sample into the tube pre-filled with sample extraction buffer. The collected fecal sample may be transported at ambient temperature, stored at room temperature or 2-8 °C for 14 days. This fecal sample may be stored below -20 °C for a 1 year and is stable minimum with three freeze - thaw cycles.

The validation data of this test were generated by using [Fecal Sample Collection Tube \(Cat. No. 30356\)](#)! To order this tube, please order [Fecal Calprotectin/NGAL Sample Collection kit \(Cat. No. KT-843\)](#). Each kit contains 50 tubes filled with extraction buffer. A different fecal NGAL test result may be obtained by using a different type of fecal sample collection tube.

2. It is an alternative to collect fecal sample with a commercial stool sample collection device. The collected sample can be stored at 2-8°C for up to 6 days. The collected sample should be diluted in two steps with 1:40 and 1:90 before measurement.

EDI Kit insert: NGAL ELISA/V5/CE/2014-10

Following is a detailed sample extraction process.

- (a) Label and tare an empty polypropylene tube together with a inoculation loop.
- (b) Weigh 50 – 100 mg of stool using the inoculation loop by placing it into the pre-tared tube.
- (c) Record the net amount of sample and break the inoculation loop; leave the lower part of the loop in the tube.
- (d) Add diluted Extraction Buffer (39 parts of the stool volume, 1 g stool = 1 ml) into the tube:

Fecal Sample Weight (mg)	Extraction Buffer Volume (ml)
50	2.0
55	2.2
60	2.4
65	2.6
70	2.8
75	3.0
80	3.2
85	3.4
90	3.6
95	3.8
100	4.0

- (e) Vortex to dissolve stool sample. Let the sample set at room temperature vertically for 30 min for sedimentation or centrifuge the sample at 3000 x g for 5 minutes.
- (f) Transfer 0.015 mL clear supernatant (no particles) to a clean tube with 1.35 ml Extraction Buffer. Mix the sample by gently vortexing. This extracted sample is ready to be measured for fecal NGAL.

ASSAY PROCEDURE

1. Reagent Preparation

- (1) Prior to use allow all reagents to come to room temperature. Reagents from different kit lot numbers should not be combined or interchanged.
- (2) ELISA Wash Concentrate (Cat. 10010) must be diluted to working solution prior to use. Please see REAGENTS section for details.
- (3) Reconstitute assay standards and controls by adding **1.0 mL** of demineralized water to each standard and control bottle. Allow the standard and controls to sit undisturbed for 5 minutes, and then mix well by inversions or gentle vortexing. Make sure that all solid is dissolved completely prior to use. These reconstituted standards and controls may be stored at 2- 8°C for up to 3 days or below -20 °C for long-term storage. Do not exceed 3 freeze-thaw cycles
- (4) Place a sufficient number of Anti-NGAL antibody-coated microwell strips (Cat. 30641) in a holder to run human NGAL standards, controls and unknown samples in duplicates.
- (5) Prepare Tracer Antibody working solution by 1:21 fold dilution of the NGAL Tracer Antibody (Cat. 30650) by adding the tracer antibody into the Tracer Antibody Diluent (Cat. 30651). Following is a table that outlines the relationship of strips used and antibody mixture prepared.

NOTE: the tracer antibody should be prepared just prior to the end of the first incubation cycle.

Dilution Scheme	Tracer Antibody Diluent	Tracer Antibody
1	1 mL	50 µL
2	2 mL	100 µL
3	3 mL	150 µL
4	4 mL	200 µL
5	5 mL	250 µL
6	6 mL	300 µL
7	7 mL	350 µL
8	8 mL	400 µL
9	9 mL	450 µL
10	10 mL	500 µL
11	11 mL	550 µL
12	12 mL	600 µL

(6) Test Configuration

ROW	STRIP 1	STRIP 2	STRIP 3	STRIP 4
A	STD 1	STD 5	SAMPLE 1	SAMPLE 5
B	STD 1	STD 5	SAMPLE 1	SAMPLE 5
C	STD 2	STD 6	SAMPLE 2	SAMPLE 6
D	STD 2	STD 6	SAMPLE 2	SAMPLE 6
E	STD 3	C 1	SAMPLE 3	
F	STD 3	C 1	SAMPLE 3	
G	STD 4	C 2	SAMPLE 4	
H	STD 4	C 2	SAMPLE 4	

2. Patient Sample Preparation:

- Patient samples collected with Fecal Sample Collection Tube (Cat. No. 30356).
All patient samples should be diluted 1:10 with 1x Calprotectin/NGAL Sample Extraction Buffer. For example, mixing 100 µl sample with 900 µl buffer in a clean test tube. This diluted sample can be used directly in the assay procedure.
- Patient samples collected and extracted according to the specimen collection section #2.
These samples don't require any further dilution and can be used directly in the assay procedure.

3. Assay Procedure:

- Add **100 µl** of Standards, Controls and diluted patient samples (diluted beforehand with NGAL Sample Dilution Buffer, **Cat. 30757**) into the designated microwells.
- Seal the plate wells securely, cover with foil or other material to protect from light. Incubate the plate static, at room temperature for **1 hr. ± 5 minutes**.
- Just prior to the end of the incubation time, dilute the proper amount of Tracer Antibody for the assay.
- Wash each well 5 times by dispensing 350 µL of working wash solution into each well and then completely

aspirating the contents. Alternatively, an automated microplate washer can be used.

- Add **100 µL** of the above Tracer Antibody to each well.
- Seal the plate wells securely, cover with foil or other material to protect from light. Incubate the plate static, at room temperature for **30 minutes ± 5 minutes**.
- Wash each well 5 times by dispensing 350 µL of working wash solution into each well and then completely aspirating the contents. Alternatively, an automated microplate washer can be used.
- Add **100 µL** of ELISA HRP Substrate (Cat. 10020) into each of the wells.
- Cover the plate with aluminum foil or other material to avoid exposure to light. Incubate the plate static, at room temperature for **20 minutes**.
- Immediately add **100 µL** of ELISA Stop Solution (Cat. 10030) into each of the wells. Mix gently.
- Read the absorbance at 450 nm with reference filter at 620 nm or 650 nm.

PROCEDURAL NOTES

- It is recommended that all standards, controls and unknown samples be assayed in duplicate. The average absorbance reading of each duplicate should be used for data reduction and the calculation of results.
- Keep light-sensitive reagents in the original amber bottles.
- Store any unused antibody-coated strips in the foil zipper bag with desiccant to protect from moisture.
- Careful technique and use of properly calibrated pipetting devices are necessary to ensure reproducibility of the test.
- Incubation times or temperatures other than those stated in this insert may affect the results.
- Avoid air bubbles in the microwell as this could result in lower binding efficiency and higher CV% of duplicate reading.
- All reagents should be mixed gently and thoroughly prior to use. Avoid foaming.
- If adapting this assay to automated ELISA system such as DS-2 (Diamedix Corp., Miami), a procedural validation is necessary if there is any modification of the assay procedure.

INTERPRETATION OF RESULTS

It is recommended to use a point-to-point or 4-parameter standard curve fitting.


- Calculate the average absorbance for each pair of duplicate test results.
- Subtract the average absorbance of the level 1 standard (0 µg/g) from the average absorbance of all other readings to obtain corrected absorbance.
- The standard curve is generated by the corrected absorbance of all standard levels on the ordinate against the standard concentration on the abscissa using point-to-point or log-log paper. Appropriate computer assisted data reduction programs may also be used for the calculation of results.

The human NGAL concentrations for the controls and the patient samples are read directly from the standard curve using their respective corrected absorbance.

EXAMPLE DATA AND STANDARD CURVE

A typical absorbance data and the resulting standard curve from this Fecal NGAL ELISA are represented. **This curve should not be used in lieu of standard curve generated with each assay.**

Well I.D.	OD 450/650 nm Absorbance			Results
	Readings	Average	Corrected	
Std-1: 0 µg/g	0.017 0.017	0.017	0.000	
Std-2: 1.2 µg/g	0.106 0.102	0.104	0.087	
Std-3: 3.6 µg/g	0.256 0.252	0.254	0.237	
Std-4: 10.8 µg/g	0.679 0.694	0.687	0.670	
Std-5: 32.4 µg/g	1.597 1.614	1.605	1.588	
Std-6: 97.2 µg/g	2.810 2.881	2.846	2.829	
Control 1	0.491 0.446	0.468	0.451	7.2 µg/g
Control 2	1.245 1.257	1.251	1.234	24 µg/g

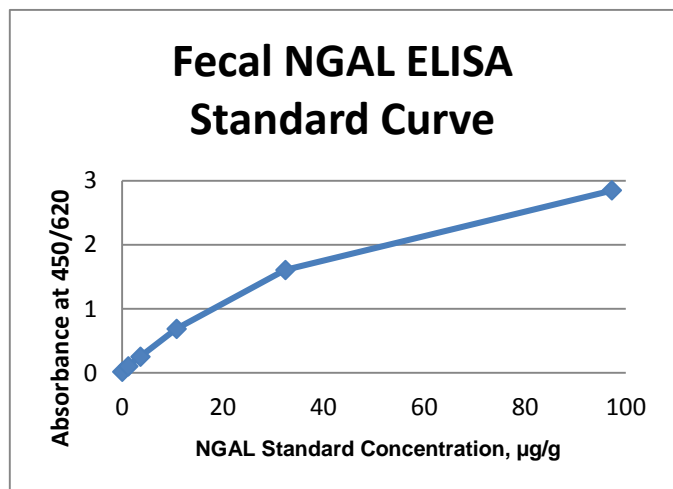

EXPECTED VALUES

Stool samples from normal healthy adults with age of 24 – 58 were collected and measured with this ELISA. The recommended normal cut-off for fecal NGAL concentration by using this ELISA and sample collection system is 25 µg/g directly read from assay standard curve. We strongly recommend that each clinical laboratory to establish its own normal cut-off level by measuring normal stool samples with this ELISA and sample collection system.

Please be aware that patients with recent diarrhea might give a much higher level of fecal NGAL. Taking spicy food or alcohol may also cause intestinal irritation resulting in an abnormal fecal NGAL level.

Note: NGAL ng/mL X 3.6 = NGAL µg/g stool
 NGAL µg/g stool X 0.278 = NGAL ng/mL

LIMITATION OF THE PROCEDURE

1. An abnormally high NGAL test result cannot be independently used for clinical diagnosis. The same as other laboratory tests, a verity of analytical and pre-

EDI Kit insert: NGAL ELISA/V5/CE/2014-10

analytical factors may lead to false high test results. Physicians must interpret the test result in the light of each patient's clinical findings.

2. For sample values reading greater than the highest standard, it is recommended to re-assay samples with further dilutions (i.e. 1:10 or 1:100 with NGAL Sample Extraction Buffer).
3. Water deionized with polyester resins may inactivate the horseradish peroxidase enzyme.

QUALITY CONTROL

To assure the validity of the results each assay should include adequate controls.

PERFORMANCE CHARACTERISTICS

Sensitivity

The analytical sensitivity (LLOD) of the NGAL ELISA as determined by the 95% confidence limit on 16 duplicate determination of zero standard is approximately 0.04 µg/g.

High Dose "hook" effect

This assay has showed that it did not have any high dose "hook" for NGAL levels up to 64,800 µg/g.

Precision

The intra-assay precision was validated by measuring three control fecal samples with 16 replicate determinations.

Sample #	Mean NGAL Value (µg/g)	CV (%)
1	3.1	3.5
2	8.0	7.4
3	23.4	4.3

The inter-assay precision was validated by measuring two control levels in duplicate in 14 individual assays.

Sample #	Mean NGAL Value (µg/g)	CV (%)
1	7.3	5.3
2	22.0	4.6

Linearity

Three stool samples were collected, spiked with various amounts of NGAL, diluted with Calprotectin/NGAL Extraction Buffer and tested. The results of NGAL percent recovery value in µg/g are as follows:

DILUTION	OBSERVED VALUE (µg/g)	% Recovery
NEAT A	4.1	-
1:2	2.0	100.1%
1:4	1.0	99.4%
1:8	0.5	99.4%
NEAT B	2.7	-
1:2	1.3	95.2%
1:4	0.7	102.7%
1:8	0.3	100.0%
NEAT C	3.1	-
1:2	1.5	97.8%
1:4	0.8	97.3%
1:8	0.4	95.0%



Distribuito in ITALIA da
Li StarFish S.r.l.
 Via Cavour, 35
 20063 Cernusco S/N (MI)
 telefono 02-92150794
 fax 02-92157285
 info@listarfish.it
 www.listarfish.it

Spike Recovery

Three stool samples and four assay standards (1.2, 3.6 and 10.8, 3.2 µg/g) were combined at equal volumes and tested. The results are as follows:

samples	OBSERVED VALUE	% RECOVERY
Neat A	0.14	-
Std-2: 1.2 µg/g	0.6	87.8%
Std-3: 3.6 µg/g	1.7	88.6%
Std-4: 10.8 µg/g	5.1	93.3%
Std-5: 32.4 µg/g	15.8	97.1%
Neat B	0.3	-
Std-2: 1.2 µg/g	0.7	90.0%
Std-3: 3.6 µg/g	1.7	88.0%
Std-4: 10.8 µg/g	4.8	87.5%
Std-5: 32.4 µg/g	13.8	84.7%
Neat C	0.2	-
Std-2: 1.2 µg/g	0.6	80.7%
Std-3: 3.6 µg/g	1.7	88.0%
Std-4: 10.8 µg/g	4.6	83.0%
Std-5: 32.4 µg/g	14.2	87.0%

This product is developed and manufactured by



EpiTope Diagnostics, Inc.
 7110 Carrol Road
 San Diego, CA 92121, USA



MDSS GmbH
 Schiffgraben 41
 30175 Hannover, Germany

Manufacturer	No. of tests
Catalog Number	Keep away from heat and direct sun light
Concentrate	Store at
In Vitro Diagnostic Device	Use by
Read instructions before use	Lot No.
Authorized Representative In Europe	

WARRANTY

This product is warranted to perform as described in its labeling and literature when used in accordance with all instructions. EpiTope Diagnostics, Inc. DISCLAIMS ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE, and in no event shall EpiTope Diagnostics, Inc. be liable for consequential damages. Replacement of the product or refund of the purchase price is the exclusive remedy for the purchaser. This warranty gives you specific legal rights and you may have other rights, which vary from state to state.

REFERENCES

- Kjeldsen L, Johnsen AH, Sengeløv H, Borregaard N (May 1993). "Isolation and primary structure of NGAL, a novel protein associated with human neutrophil gelatinase". *J. Biol. Chem.* **268** (14): 10425–32.
- Chan P, Simon-Chazottes D, Mattei MG, Guenet JL, Salier JP (September 1994). "Comparative mapping of lipocalin genes in human and mouse: the four genes for complement C8 gamma chain, prostaglandin-D-synthase, oncogene-24p3, and progesterone-associated endometrial protein map to HSA9 and MMU2". *Genomics* **23**(1): 145–50.
- Cowland JB, Borregaard N (October 1997). "Molecular characterization and pattern of tissue expression of the gene for neutrophil gelatinase-associated lipocalin from humans". *Genomics* **45** (1): 17–23.
- Yang J, Goetz D, Li JY, Wang W, Mori K, Setlik D, Du T, Erdjument-Bromage H, Tempst P, Strong R, Barasch J (November 2002). "An iron delivery pathway mediated by a lipocalin". *Mol. Cell* **10** (5): 1045–56.
- Friedl A, Stoesz SP, Buckley P, Gould MN (July 1999). "Neutrophil gelatinase-associated lipocalin in normal and neoplastic human tissues. Cell type-specific pattern of expression". *Histochem. J.* **31** (7): 433–41.

NGAL ELISA: Condensed Assay Protocol

- 100 µl Standards, controls, and diluted patient samples

Incubate @ RT for 60 min
 static
 Wash 5 x



- 100 µl Tracer Antibody

Incubate @ RT for 30 min
 static
 Wash 5 x



- 100 µl TMB Substrate

Incubate @ RT for 20 min
 static



- 100 µl Stop Solution

Immediately



- Read absorbance at 450/650 or 450/620 nm

within 10 minutes