



# MONOSCREEN<sup>®</sup> Ab ELISA

## BRSV

ELISA kit for serodiagnosis of Bovine Respiratory Syncytial Virus (BRSV)

Indirect test for blood sera, plasma and milk

Diagnostic test for cattle

Double wells

### ***I - INTRODUCTION***

In Europe, BRSV is the most important etiological agent responsible for respiratory affections in young cattle. In cattle as in children, respiratory syncytial viruses can cause a very deep attack of the respiratory tree. The affection is often provoking very severe injuries, which are responsible for important economical losses. As a matter of fact, in Europe, 7 million calves suffer from infections diseases yearly, 60 % of which are caused by respiratory pathogens. One million calves are dying each year of respiratory diseases in the European Community. The cost of these diseases which includes medical treatments, growth delays and mortality is about 450 millions EURO per year for calves under one year. For dairy cattle, the cost of BRSV has been evaluated at around 25 EURO per animal.

BRSV is principally affecting young cattle. Beef cattle is especially vulnerable because of the muscular mass of the animal which is very important compared to the pulmonary volume. Clinical manifestations can be dramatic. Often signs of severe pneumonia such as polypnea, abdominal breabbling and hyperthermia are present. Reinfections can be observed but most often they remain subclinical. Clinical diagnosis is very difficult and laboratory assistance is required for a precise diagnosis. Virus can be detected in lung tissue by fluorescein labelled specific antibodies.

Diagnosis can also be achieved by measuring a virus specific seroconversion. To do so, a first sample will be collected during the acute phase of the disease and a second sample will be collected 2 or 3 weeks later.

These two samples will be evaluated for their content in specific antibodies against BRSV by ELISA.

### ***II – PRINCIPLE OF THE TEST***

The test uses 96-well microtitration plates sensitised by monoclonal antibodies specific to F protein of BRSV virus. This antibody is used to trap a recombinant F protein. The plate's odd columns (1, 3, 5, 7, 9 and 11) contain the recombinant viral protein, whereas the even columns (2, 4, 6, 8, 10 and 12) contain a control antigen. We thus have a genuine negative control to differentiate the specific anti- viral antibody from the antibodies directed against the control antigen. Using such a control reduces the number of false positives considerably.

The test blood sera, plasma or milks are diluted in the dilution buffer. Samples are added to the plate which is then incubated and washed. The conjugate, a peroxidase-labelled anti-bovine IgG1 monoclonal antibody, is added to the wells. The plate is then incubated a second time at 21°C +/- 3°C and washed again and the chromogen (tetramethylbenzidine) is added. This chromogen has the advantage of being more sensitive than the

other peroxidase chromogens and not being carcinogenic. If specific BRSV immunoglobulins are present in the test sera the conjugate remains bound to the microwell that contains the viral antigen and the enzyme catalyses the transformation of the colorless chromogen into a pigmented compound. The intensity of the resulting blue colour is proportionate to the titre of specific antibody in the sample. The signal read off the negative control microwell is subtracted from that of the positive microwell sensitised by the viral antigen. It is possible to quantify the reactivity of an unknown sample on a scale ranging from 0 to +++++.

### III - COMPOSITION OF THE KIT

- **Microplates:** 96-well microtitration plates. The odd columns (1, 3, 5, 7, 9 and 11) are sensitised by the recombinant F protein from BRSV and the even columns (2, 4, 6, 8, 10 and 12) by the control antigen.
  - **Washing solution:** One bottle of 20x concentrated washing solution. The solution crystallises spontaneously when cold. If only part of the solution is to be used, bring the bottle to 21°C +/- 3°C so that all the crystals disappear. Mix the solution well and remove the necessary volume. Dilute the buffer 1:20 with distilled or demineralised water.
  - **Dilution buffer:** One bottle of 5x colored, concentrated buffer for diluting blood sera, plasma, milks and conjugate. The bottle's content is to be diluted with distilled or demineralised water. If a deposit forms at the bottom of the receptacle filter the solution on Whatman filter paper.
  - **Conjugate:** 1 bottle of anti-bovine immunoglobulin-peroxidase conjugate (horseradish peroxidase-labelled anti-bovine IgG1 monoclonal antibody).
  - **Positive reference:** One bottle of positive serum. Store this reagent between +2°C and +8°C.
  - **Negative reference:** One bottle of negative serum. Store this reagent between +2°C and +8°C.
  - **Tracer :** One bottle of tracer. The tracer is a reference sample that can be used to check the intra-laboratory reproducibility of the kit's batch.
- Intra-laboratory reproducibility:** Degree of agreement between the results of reiterated tests on the same sample with an identical technical protocol in a given laboratory under variable working conditions.
- **Single component TMB:** One bottle of the chromogen tetramethylbenzidine (TMB). Store between +2°C and +8°C protected from the light.
  - **Stop solution:** One bottle of the 1 M phosphoric acid stop solution.

	BIO K 061/2	BIO K 061/5
Microplates	2	5
Washing solution	1 X 100 ml (20 X)	1 X 250 ml (20 X)
Colored Dilution buffer	1 X 50 ml (5 X)	1 X 100 ml (5X)
Conjugate	1 X 0,5 ml (50 X)	1 X 1,4 ml (50 X)
Positive serum	1 X 0,5 ml (1 X)	1 X 0,5 ml (1 X)
Negative serum	1 X 0,5 ml (1 X)	1 X 0,5 ml (1 X)
Tracer	1 X 0,5 ml (1 X)	1 X 0,5 ml (1 X)
Single component TMB	1 X 25 ml (1 X)	1 X 55 ml (1 X)
Stop solution	1 X 15 ml (1 X)	1 X 30 ml (1X)

### IV - ADDITIONAL MATERIALS AND EQUIPMENT REQUIRED

Distilled water, graduated cylinders, beakers, plastic tubes, tube rack, microplates for dilution, dispenser tips, reagent reservoir for multichannel pipettes, lid, adhesive for microplates, graduated automatic (mono- and multichannel) pipettes, microplate reader, and microplate washer and shaker (optional)

### V - PRECAUTIONS FOR USE

- This test may be used for "in vitro" diagnosis only. It is strictly for veterinary use.
- The reagents must be kept between +2°C and +8°C. The reagents cannot be guaranteed if the shelf-life dates have expired or if they have not been kept under the conditions described in this insert.
- The concentrated wash solution and dilution buffer may be stored at room temperature. Once diluted, these solutions remain stable for six weeks if kept between +2°C and +8°C.
- Unused strips must be stored immediately in the aluminium envelope, taking care to keep the desiccant dry and the envelope's seal airtight. If these precautions are taken, the strips' activity can be conserved up to the kit's shelf-life date.
- Do not use reagents from other kits.

- The quality of the water used to prepare the various solutions is of the utmost importance. Do not use water that may contain oxidants (e.g., sodium hypochlorite) or heavy metal salts, as these substances can react with the chromogen.
- Discard all solutions contaminated with bacteria or fungi.
- The stop solution contains 1 M phosphoric acid. Handle it carefully.
- All materials and disposable equipment that come in contact with the samples must be considered potentially infectious and be disposed of in compliance with the legislation in force in the country.
- To guarantee the reliability of the results, one must follow the protocol to the letter. Special care must be taken in observing the incubation times and temperatures, as well as measuring the volumes and dilutions accurately.

## **VI – PROCEDURE**

1- Bring all components to 21°C +/- 3°C before use. Remove the microplate from its wrapper.

### 2- DILUTION OF SAMPLES

#### *2.1- Blood sera and plasma preparation*

The blood serum and plasma samples must be diluted 1:100. Avoid using haemolysed samples or those containing coagulum.

##### *2.1.1- Dilution in tubes*

Distribute 990 µl aliquots of dilution buffer, prepared as instructed in the section “Composition of the Kit”, to 5 or 10 ml tubes. Add 10 µl aliquots of the samples to each of these tubes and mix briefly on a mechanical stirrer (final dilution: 1:100).

##### *2.1.2- Dilution on a microplate*

Distribute 20 µl aliquots of each of the samples to the microwells of a dilution plate. Add 180 µl of dilution buffer. Mix five times by pumping and surging or orbital agitation (dilution: 1:10). Distribute 90 µl aliquots of dilution buffer to the wells of the kit’s microplate. Transfer 10 µl of the 1:10 prediluted samples. Mix five times by pumping and surging or orbital agitation (final dilution: 1:100).

#### *2.2- Dilution of the kit’s reference sera (positive and negative controls) and tracer*

The positive and negative sera and the tracer must be diluted 1:100. Do these dilutions in one step in a tube (see Point 2.1.1.) or in two steps on a dilution microplate (see Point 2.1.2.).

#### *2.3- Milk preparation*

Centrifuge at 4000 g for 20 minutes. Take up the middle layer of liquid by means of a glass Pasteur pipette inserted through the upper layer of cream, taking care not to touch the underlying cell sediment.

The milk samples must be diluted 1:4.

##### *2.3.1- Dilution in tubes*

Distribute 750 µl aliquots of dilution buffer, prepared as instructed in the section “Composition of the Kit”, to 5 or 10 ml tubes. Add 250 µl aliquots of milk to each of these tubes and mix briefly on a mechanical stirrer (final dilution: 1:4).

##### *2.3.2- Dilution on a microplate*

Distribute 60 µl of each sample to the microwells of a dilution plate. Add 180 µl of dilution buffer. Mix five times by pumping and surging or orbital agitation (dilution: 1:4). Transfer 100 µl aliquots of the diluted samples to the kit’s microplate.

3- Distribute the samples (blood serum, plasma, or milk) using 100 µl per well. For example, the following pattern may be followed: Positive serum in wells A1 and A2, Negative serum in wells B1 and B2, Tracer in wells C1 and C2, Sample 1 in wells D1 and D2, and so on. Cover with a lid and incubate the plate at 21°± 3°C for one hour.

4- Rinse the plate with the washing solution prepared as instructed in the section “Composition of the Kit”. To do this, dispose of the microplate’s contents by flipping it sharply over a container filled with an inactivating agent. Let the microplate drain upside-down on a sheet of clean absorbent paper so as to eliminate all liquid. Add 300 µl of the washing solution, and then empty the plate once again by flipping it over above the

containment vessel. Repeat the entire operation two more times, taking particular care to avoid bubble formation in the wells. After these three rinses, go on to the next step.

Using a plate washer (whether automatic or manual) is also recommended. However, the depth of the needles' immersion must be set so as not to disturb the layer of reagents adsorbed to the bottom of each well.

- 5- Dilute the conjugate 1:50 in the dilution buffer (for example, for one plate dilute 250 µl of the conjugate stock solution in 12.250 ml of diluent). Add 100 µl of the diluted conjugate solution to each well. Cover the plate with a lid and incubate the plate at 21°± 3°C for one hour.
- 6- Wash the plate as described in step 4 above.
- 7- Add 100 µl of the chromogen solution to each well on the plate. The chromogen solution must be absolutely colourless when it is pipetted into the wells. If a blue colour is visible, this means that the solution in the pipette has been contaminated.
- 8- Incubate for 10 minutes at 21°C +/- 3°C protected from the light and uncovered. This time is given as a guideline only, for in some circumstances it may be useful to lengthen or shorten the incubation time.
- 9- Add 50 µl of stop solution per microwell. The blue colour will change into a yellow colour.
- 10- Read the optical densities in the microwells using a plate reader and a 450 nm filter. Results must be read fairly soon after the stopping solution has been added since the chromogen may crystallize in wells with strong signals and thereby distort the data.

## VII – INTERPRETING THE RESULTS

Subtract from each value recorded for the odd columns the signal of the corresponding negative control well and write down the result. In performing this calculation, allow for any negative values that may exist. Carry out the same operations for the column corresponding to the positive control.

The test can be **validated** only if the positive control serum yields a difference in optical density at 10 minutes that is greater than 0,800 and the negative control serum yields a difference in optical density that is lower than 0,300

Divide the signal read for each sample well by the corresponding positive control serum signal and multiply this result by 100 to express it as a percentage.

$$\text{Val(ue)} = \frac{\text{Delta OD Sample} * 100}{\text{Delta OD positive}}$$

Using the following table, determine each serum's, plasma's or milk's degree of positivity.

0		+		++		+++		++++		+++++
Val <=	20 %	< Val <=	40 %	< Val <=	60 %	< Val <=	80 %	< Val <=	100 %	< Val


A reliable diagnosis can be made only if frank seroconversion can be documented using two coupled serum samples taken at 2- to 3-week intervals. The first sample must be taken during the acute phase of the infection. A frank seroconversion is considered to have occurred if the signal increases by two orders of magnitude (two plusses; for example, ++ -> ++++ or + -> +++). A sample must be considered positive if it yields a result that is **greater than or equal to one plus sign (+)**.

## VIII – ORDERING INFORMATION

Monoscreen AbELISA BRSV

2x48 tests  
5x48 tests

BIO K 061/2  
BIO K 061/5

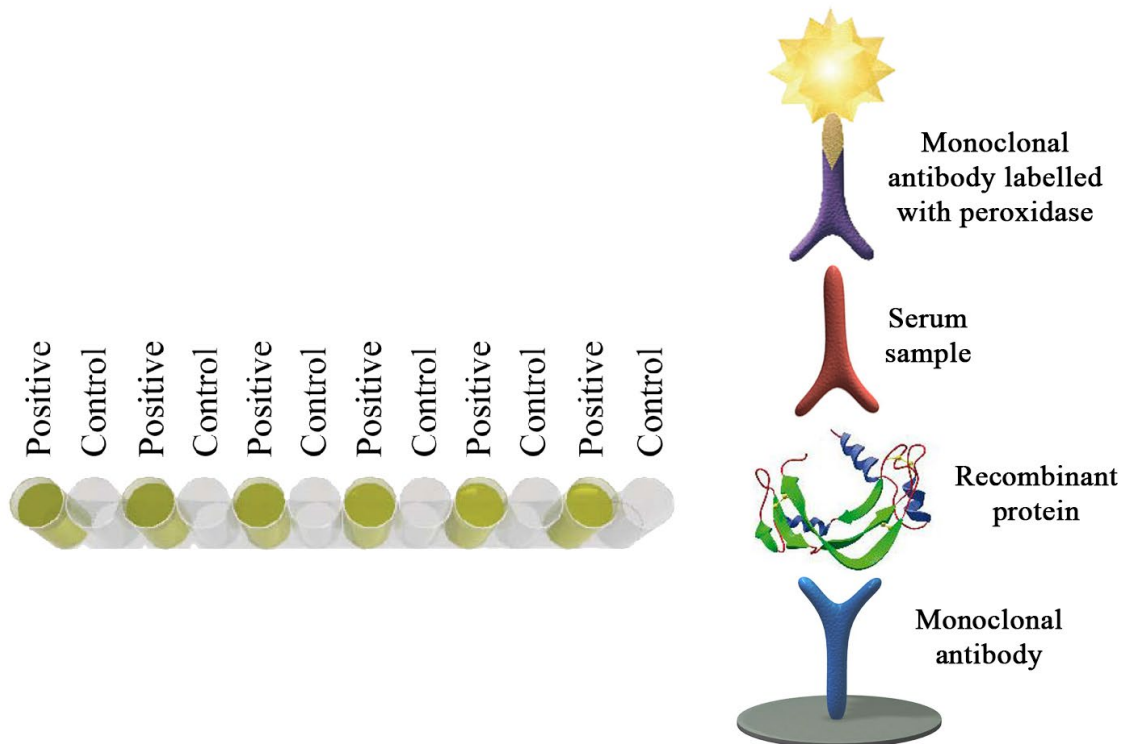

Distribuito in ITALIA da  
**Li StarFish S.r.l.**  
Via Cavour, 35  
20063 Cernusco S/N (MI)  
telefono 02-92150794  
info@listarfish.it  
www.listarfish.it